


Sure-Lok[®]

Introducing *Sure-Lok[®]*, the new Needle-Free I.V. connector in Amsino's *AMSafe[®]* product line.

The Sure-Lok[®] is designed with transparent housing, tight septum seal and smooth swab able surface to help reduce bacterial contamination and support infection control.¹ The Sure-Lok[®] has a high flow rate and a proven lower resistance to luer connections allowing ease of connection the ability to use the device easily and effectively.²

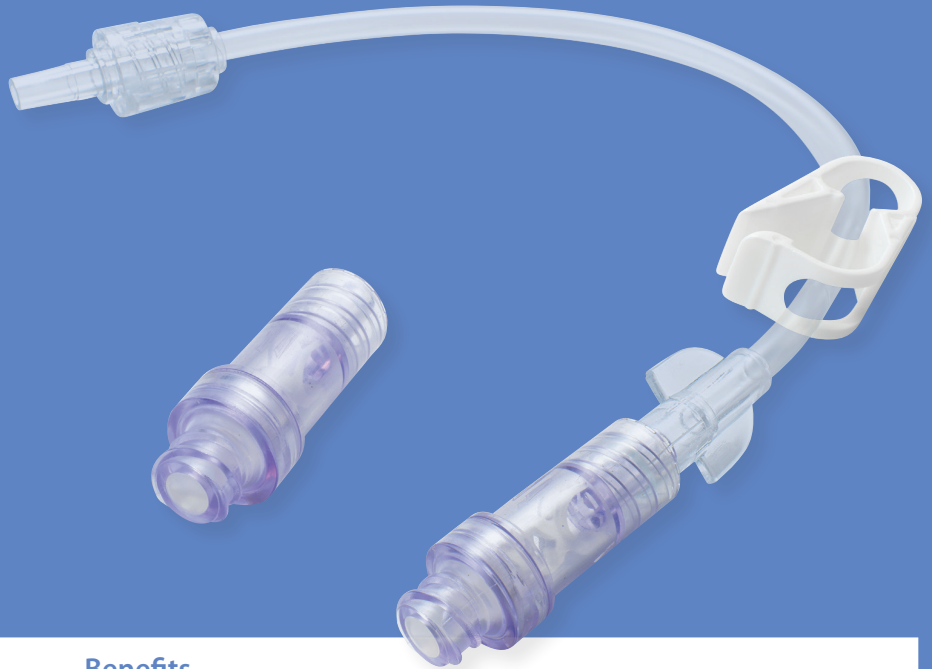

| Features | Benefits |
|--------------------------------------|--|
| Clear housing and septum | Provides a visual confirmation of fluid flush |
| Improved flow rate | Fluid delivery at a rate >200 mL/minute |
| Lower resistance to luer connections | Designed for easy connection and disconnection |
| Flat top with tight septum seal | Helps to support effective disinfection |
| Metal free | MRI compatible |

For more information, contact Amsino Customer Service
at 800.632.6746 or email: cssupport@amsino.com

Visit us online at www.amsino.com

AMSINO

Advancing Healthcare Worldwide[®]

Amsino International, Inc.

708 Corporate Center Drive, Pomona, CA 91768
800.632.6746 • fax: 909.626.3888 • info@amsino.com

SOURCES:

1. Jarvis W., MD. Choosing the Best Design for Intravenous Needleless Connectors to Prevent Bloodstream Infections. Infection Control Today, August 2010 <https://www.infectioncontroltoday.com/infusion-vascular-access/choosing-best-design-intravenous-needleless-connectors-prevent-bloodstream>
2. Amsino International, Inc. has proprietary data on file.

Product(s) described may not be licensed or available for sale in all countries. Please see the Instructions for Use/Operator's Manual for a complete listing of the indications, contraindications, warnings and precautions. The symbol ® indicates the trademark is registered in the U.S. Patent and Trademark Office and certain other countries. AMSafe and Sure-Lok are registered trademarks of Amsino International, Inc. © Copyright 2016, Amsino International, Inc. All rights reserved.